



How to Enter results for non-DOCKED devices (POCT Manual Result) for PCA's

This tip sheet explains how to manually enter Point-of-Care Testing (POCT) results for non-docked devices in Epic using the Enter/Edit Results activity and Worklist, highlighting that these results remain within Epic and do not interface to Cerner. This functionality is applicable to the following orders: Below are several Point-of-Care Testing (POCT) Manual Result tests available in Epic. Please note that this list is subject to change over time as new tests are created or existing ones are inactivated. When searching for a POCT test, use the search term 'POCT manual'

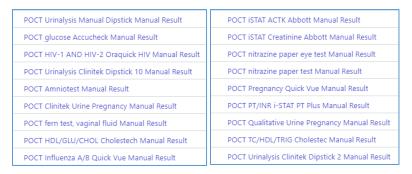


Enter/Edit Results

1. From the More Activities Drop-Down Icon, click the Enter/Edit Results Activity.




2. From the Enter/Edit Results Activity, click on the necessary POCT manual test to result.

continued...

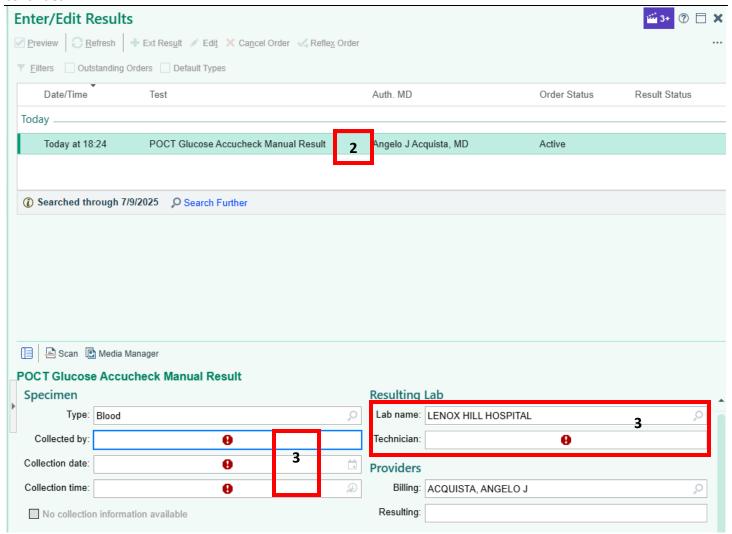

- 3. Enter specimen information. Collected by, Collection Date, Collection time and Technician are required fields. Resulting Lab, Lab Name will default to the facility the Patient is located in. NOTE: If the patient is in an outpatient location, the Lab Name will have to be manually entered.
- 4. Enter all the required result information for the test.

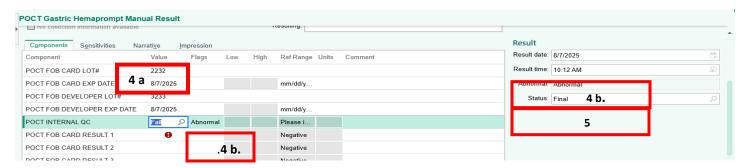

- a. Lot # can be manually entered or scanned.
- b. If value of Fail is selected in Internal QC, the system will default Abnormal in the Flags column as well as the Abnormal field under Results. **NOTE**: When correcting Results, you will need to manually clear the Abnormal flags, they will not clear automatically.
- 5. Result Status defaults to final for all Enter/Edit Results. Select Accept on the bottom right.

Enter/Edit Results from the Worklist

PCA's can also perform Enter/Edit Results from the Worklist.

1. Click on the Enter/Edit results in the Time Column



2. The Enter/ Edit Result screen appears. The same steps will apply that are listed above for steps 3, 4, 4b and 5.

